

# NON-TOUCH Infrared Thermometer JPD-FR202



1S

1 Second  
Reading

**JPD-FR202** Infrared Thermometer measures the body temperature based on the infrared energy emitted from the forehead. Users can quickly get measurement results after positioning properly the temperature probe at forehead.

## FEATURES



Professional  
Accuracy



10s Auto  
Shut Off



Hygienic  
Non-Touch



Smart  
Fever Alert



Silent Mode

## Fever warning




## Safe & Hygienic



## Multiple use




## 20 memories

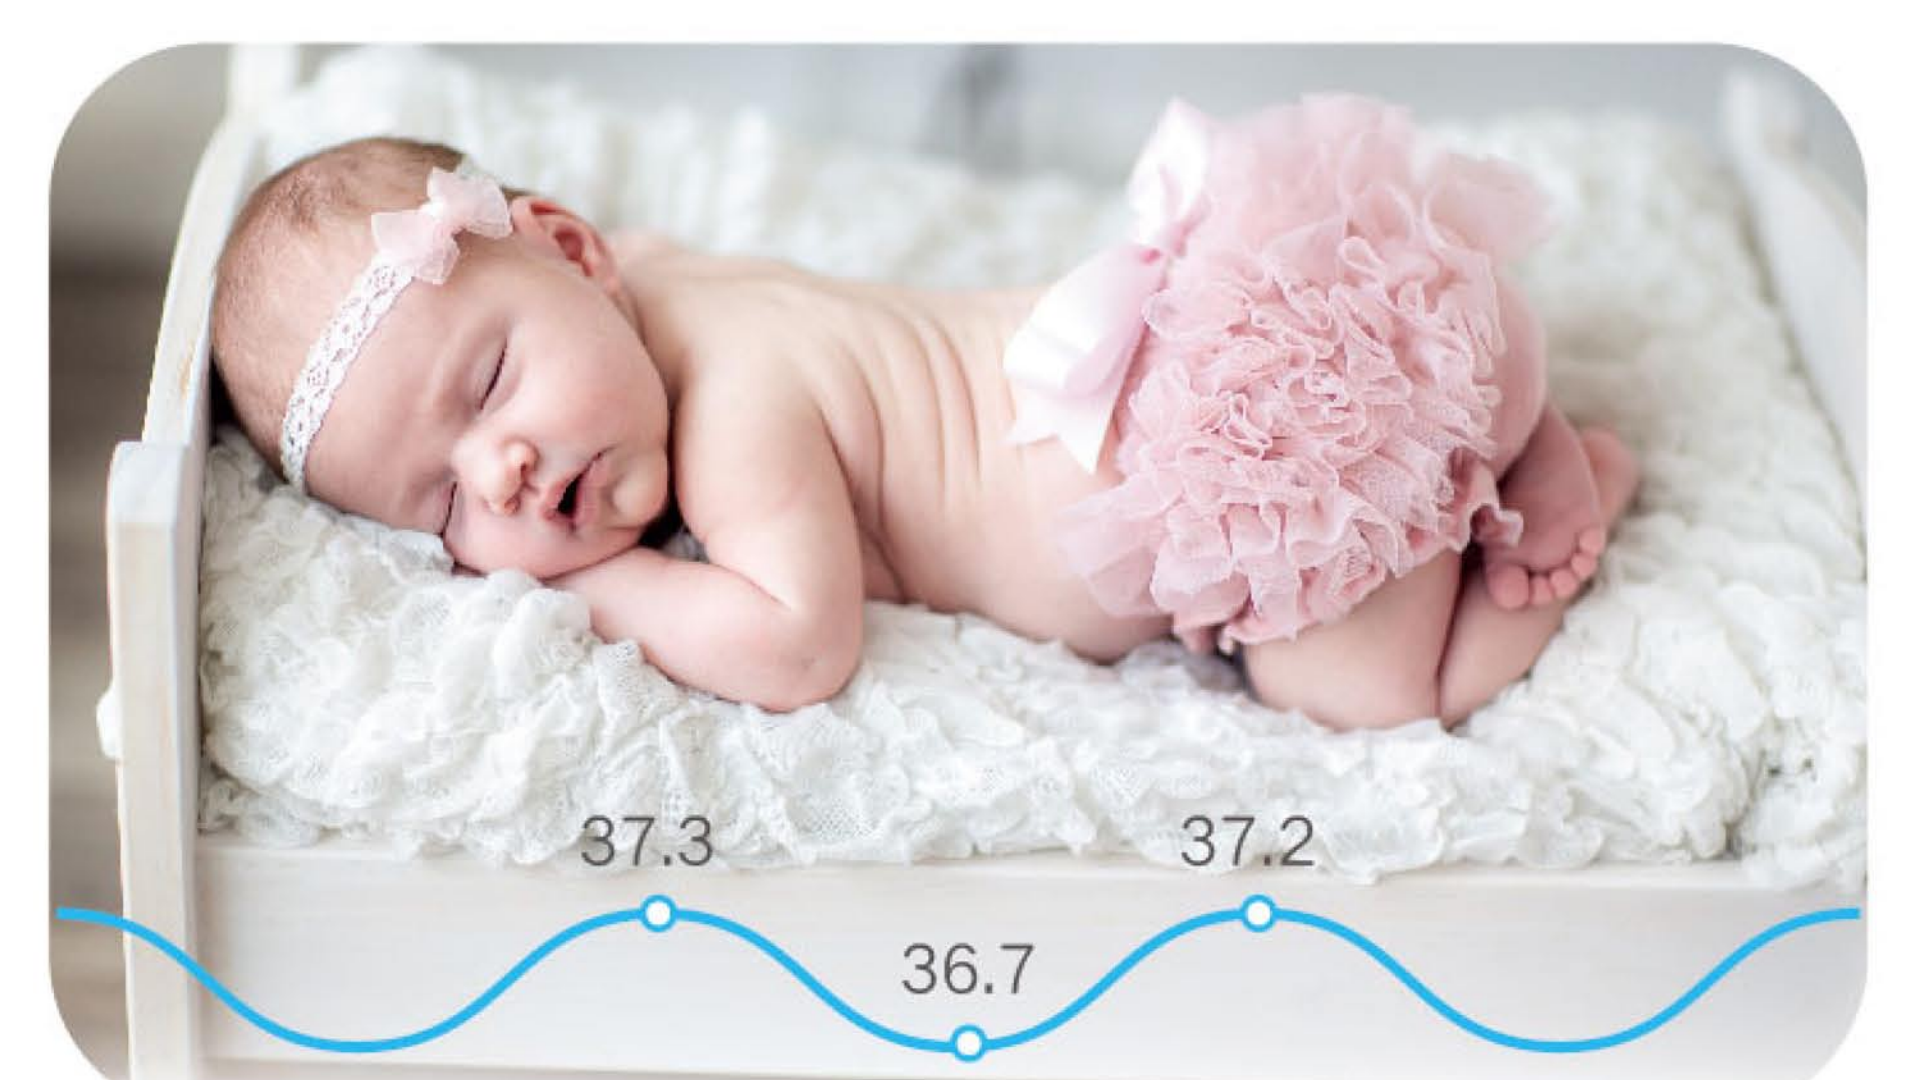




## DISPLAY DESCRIPTION

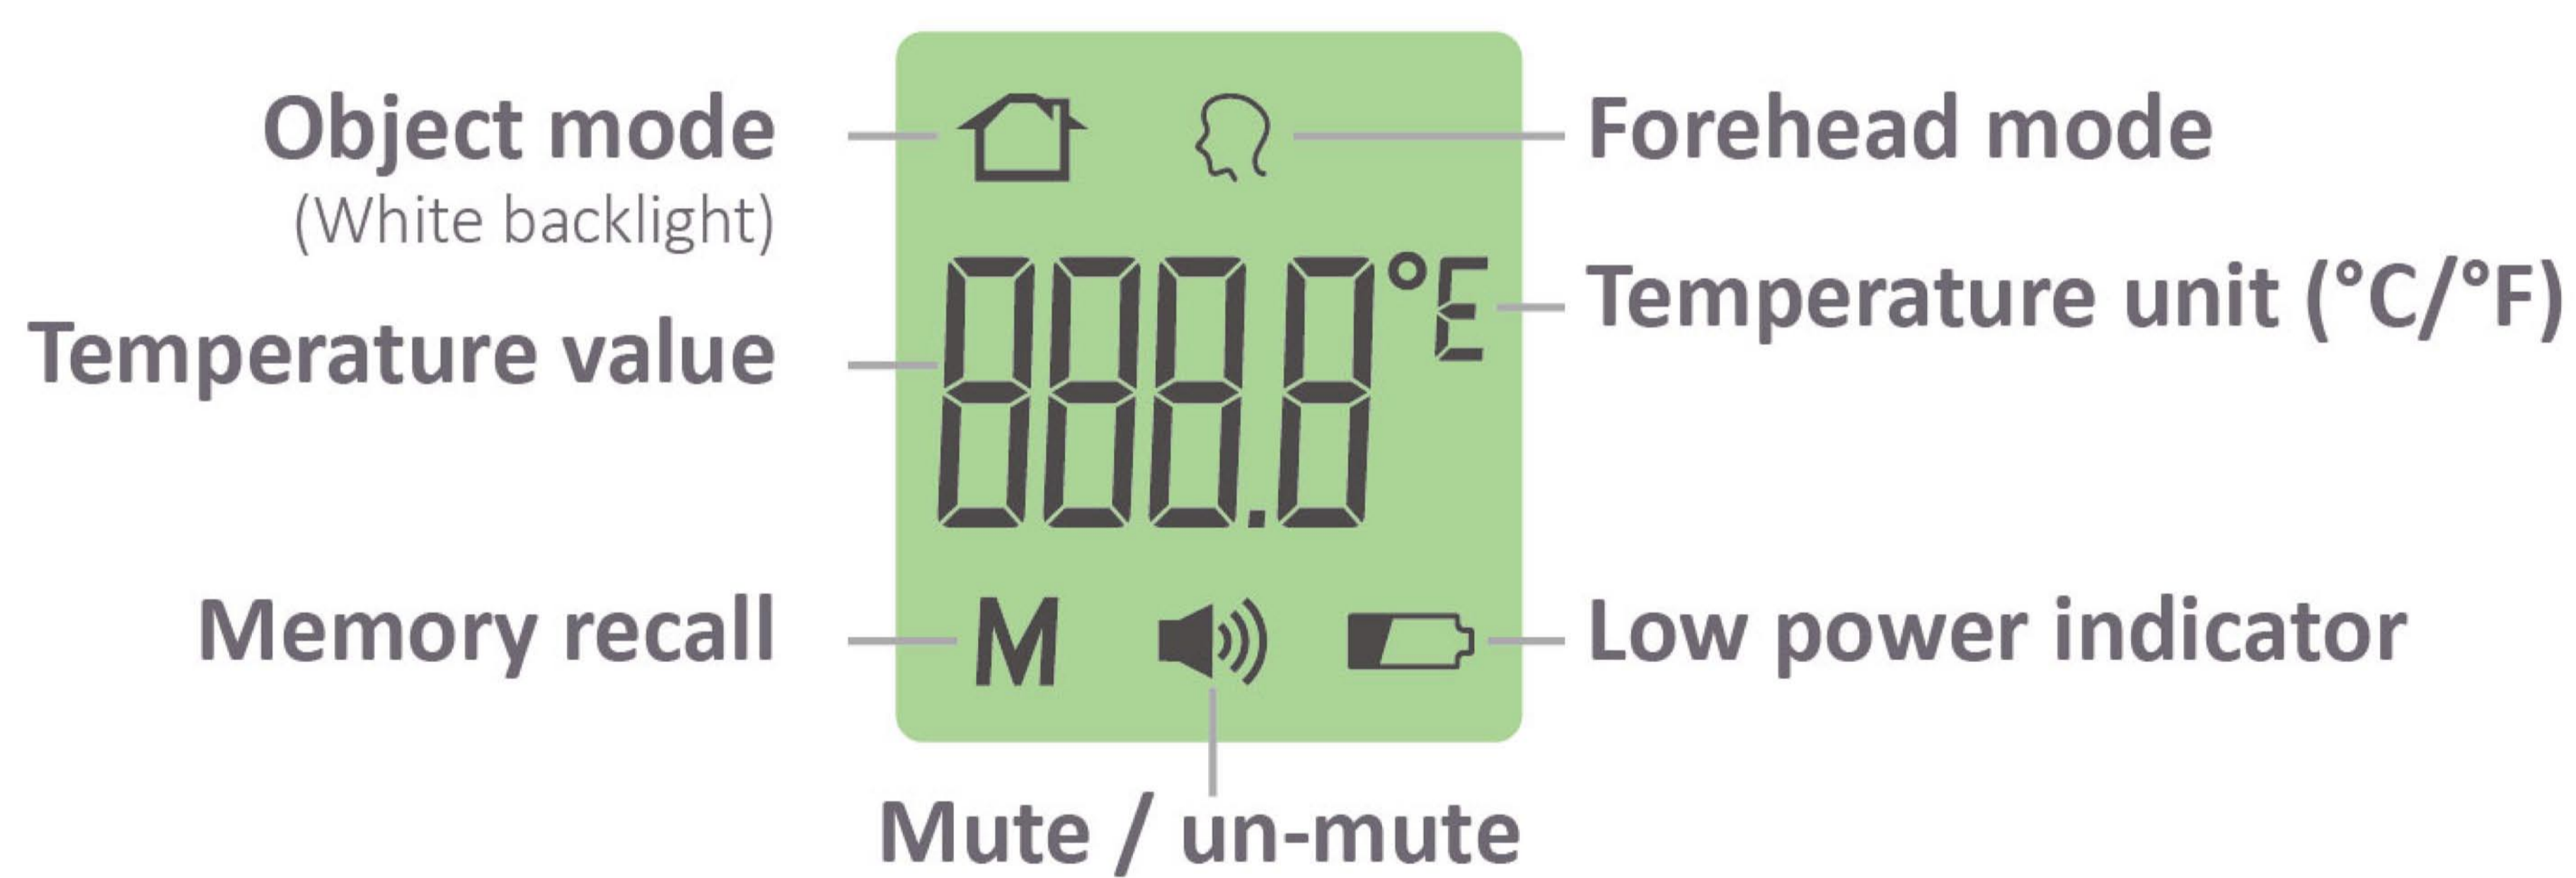

## QUICK GUIDE

1. Part hair
2. Wipe sweat
3. Point at the center (1-3cm)

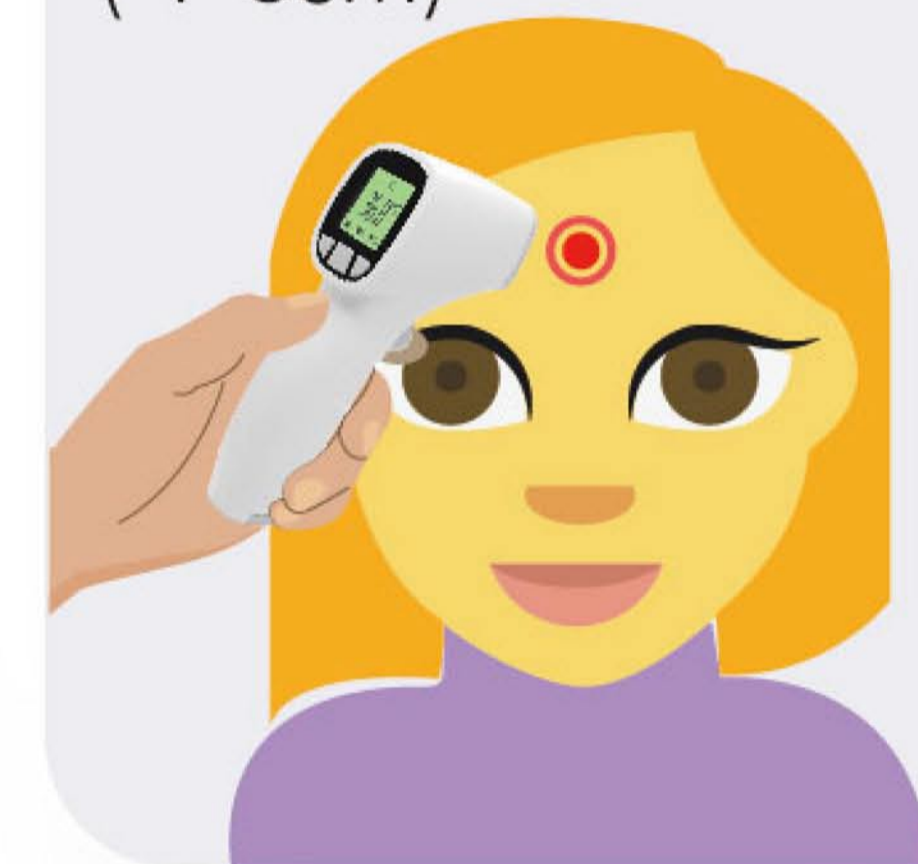

## PACKING SPECIFICATION

CTN SIZE(CM)	QTY/CTN	GW(KG)	FCL/20
47 x 34 x 28	50	9.5	560

### ACCESSORIES

Storage bag × 1  
User manual × 1

AAA batteries × 2



## SPECIFICATION

Display	HD LCD Display
Measuring range & accuracy	
Forehead mode	35-42.2°C ± 0.2°C / 95-108.0°F ± 0.4°F
Object mode	0-100.0°C ± 1.0°C / 32-212.0°F ± 2.0°F
Memory storage	20 sets of Measurement data
Temperature units	°C/°F adjustable
Automatic shutdown function	10s ± 1s
Battery	AAAx2

# EC Certificate of Conformity

## The Notified Body

**MEDCERT Zertifizierungs- und Prüfungsgesellschaft für die Medizin GmbH  
Pilatuspool 2 – 20355 Hamburg – Germany**

herewith certifies that the company:

**Shenzhen Jumper Medical Equipment Co., Ltd.  
D Building, No. 71, Xintian Road, Fuyong Street,  
Baoan, Shenzhen, Guangdong  
China**

has introduced, applies and maintains a quality assurance system for the products / product categories listed in the appendix.

The compliance of this quality assurance system with the below mentioned requirements of the **Council Directive 93/42/EEC** was verified by an audit:

## Annex II without section 4

This certification is subject to surveillance by MEDCERT.

**Effective date: 2019-12-20**

**Expiry date: 2024-05-27**

Report No.: 7111FS10F

Process No.: QS – 7111

Certificate No.: 7111GB410191220

Hamburg, 2019-12-20



MEDCERT Certification Body  
(Markus Bianchi)

The certificate is only valid when provided entirely with all of its pages.  
To verify the validity of this certificate, contact [info@medcert.de](mailto:info@medcert.de).

MEDCERT Identification Number: 0482

Form F10010005e EN / Rev. 11 / 2019.11.14



Benannt durch/Designated by  
Zentralstelle der Länder  
für Gesundheitsschutz  
bei Arzneimitteln und  
Medizinprodukten  
[www.zlg.de](http://www.zlg.de)  
ZLG-BS-237.10.15

## Appendix of EC Certificate of Conformity

Process No.: QS – 7111

Certificate No.: 7111GB410191220

### List of products / product categories included in the scope of certificate

- **Fetal dopplers**
- **Fetal/maternal monitors**
- **Multi parameter patient monitors**
- **Pulse oximeters**
- **Infrared thermometers**
- **Electronic blood pressure monitors**

– End of list –

This appendix is integral part of the above-referenced certificate.  
The certificate is only valid when provided entirely with all of its pages.  
To verify the validity of this certificate, contact [info@medcert.de](mailto:info@medcert.de).

MEDCERT Identification Number: 0482

Form F10010005e EN / Rev. 11 / 2019.11.14



Benannt durch/Designated by  
Zentralstelle der Länder  
für Gesundheitsschutz  
bei Arzneimitteln und  
Medizinprodukten [www.zlg.de](http://www.zlg.de)  
ZLG-BS-237.10.15